



PRODUCT MANUAL

Resistance temperature sensor to thermowell DIN with connecting screw-joint on adapter without converter, with converter or Ex ia design type series 230 type 236

FOR DESIGNS WITH CONVERTER A MANUAL IS ENCLOSED TO THE RELEVANT CONVERTER
FOR DESIGN WITH CONVERTER AND DISPLAY A MANUAL IS ENCLOSED TO THE RELEVANT CONVERTER AND DISPLAY

APPLICATION

- For exact remote measurement of temperature of steady and running liquids (gases and fluids), for which the properties of the thermowell of the sensor selected by the customer are suitable; measurement may be realized up to temperature (max. 600°C) and pressure determined by thermowell resistance
- For explosive conditions in areas Zone 2, Zone 1 and Zone 0 pursuant to EN 60079-10 in case of using the converter Ex ia or in case of connection to the Ex ia circuit
- In a set with control or diagnostic systems for process monitoring
- In design with converter for transfer of resistance sensor signal to unified output signal 4 to 20 mA or digital signal (converter with HART protocol)
- In design with display to display the value of the measured value
- For the environment, where mechanical resistance is required pursuant to EN 60068-2-6 (class AH2) and seismic capability of the electrical equipment of the safety system of the nuclear power stations pursuant to EN IEC/IEEE 60980-344 (SSE/S2)
- special design for cryogenic environment with medium temperature up to -269 °C

The sensors with converter and Ex ia design are rated products pursuant to the Directive 2014/30/EU of the European Parliament and the Council and EU Declaration of Conformity **EU -236000** is issued for them.

For use temperature sensors as separate assemblies of the heat meter on placing on the market.

The sensors are rated products pursuant to the Directive 2014/32 EU of the European Parliament and the Council and EU Declaration of Conformity **EU-MID-236000-EN** is issued for them.

Using sensors within the meaning of Directive 2014/32 EU of the European Parliament and the Council. (MID) as part of the customer's measurement kits, for which the conformity of the assemblies as a whole must be assessed when placed on the market with all the features required by this directive:


- sensor without transmitter in 1xPt100 /.. / 4 connection can be used by the customer on the basis of an evaluation certificate in its measuring sets in the sense of Directive 2014/32 EU of the European Parliament and the Council

DESCRIPTION

The sensor consists of a replaceable measuring insert with flange and ceramic terminal board or installed two-wire converter (insulated or non-insulated, even in design Ex i) and protective armature consisting of a head and an adapter with a screw-joint for the connection of the sensor into the thermowell selected by the customer. The head with measuring insert and gland form a fixed closure Ex d. It is provided with a lid, which can be screwed, and a cable gland for the connecting wiring. The cable gland (pursuant to the required diameter of the cable) forms optional accessories to the sensor. The terminal board (of the converter) of the sensor is accessible after removing the lid of the head, which is fixed, after being tightened, with a pin against spontaneous releasing.

The sensor with converter in design Ex ia is provided with an external clamp on the head for the connection of the grounding wire or wires for mutual interconnection.

The sensor with converter is supplied from an external source. The installed converter is pre-set to the required range at the sensor manufacturer.

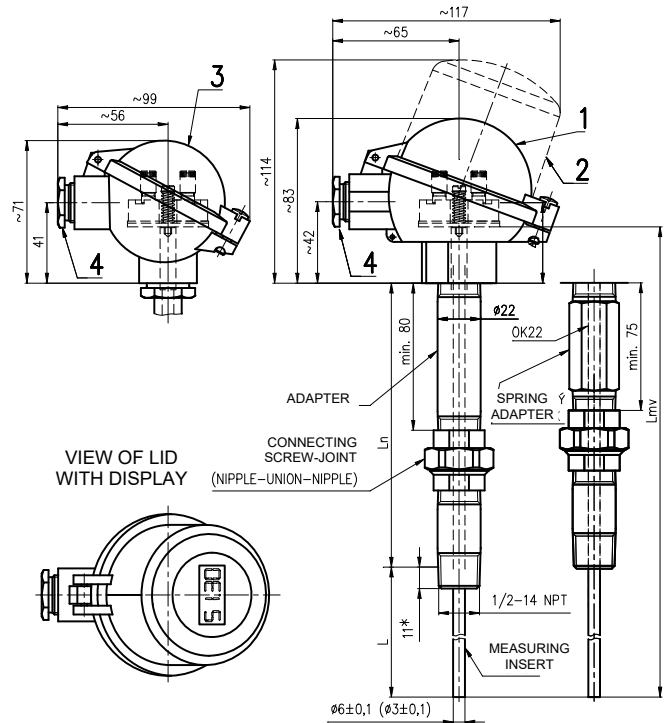

- L nominal length
- L_n length of adapter
- L_{mv} length of measuring insert (does not apply to spring adapter)
- 11* standard length of screwing

To measure temperature, a defined change of thermoelectric voltage of the sensor in dependence on the change of temperature of the measured environment is used.

TECHNICAL DATA

The sensor design is based on DIN 43772. The sensor is designed pursuant to EN 61140 as an electric equipment of protection class III for the application in networks with category of overvoltage in installation II and pollution grade 2 pursuant to EN 61010-1; the follow-up (evaluation) device shall comply with Article 6.3 of the said standard.

Measuring range:

Sensor with standard extension
 $L_n = 150$ (140) mm -70 to 600 °C *) **) -269 to 100 °C **) ***)

Sensor with shortened extension
 $L_n \text{ min} = 80$ mm -70 to 250 °C *) **) -269 to 100 °C **) ***)

*) The upper limit of the measurement range is limited by resistance of the material of the applied thermowell.

**) Class A is only guaranteed in the range from -70 to 300 °C

***) Special design for cryogenic environments

Measuring range of the sensor with converter is established by the range of the selected converter.

Electric strength pursuant to EN 61010-1, Article 6.8.3:

500 V eff (only measuring insert without converter or design with insulated converter)

Electric insulation resistance pursuant to EN IEC 60751

min. 100 M Ω , at 15 to 35°C, max. 80 % relative humidity
 min 100 V DC

Intrinsically safe pursuant to EN IEC 60079-0 and EN 60079-11:

- ⊕ II 1 G Ex ia IIC T5/T6 Ga
(Meaning of designation - see figure 3)
- P_i = 192 mW T6 (-60°C ≤ Ta ≤ 60°C)
- P_i = 290 mW T6 (-60°C ≤ Ta ≤ 55°C)
- T5 (-60°C ≤ Ta ≤ 65°C)

Intrinsically safe circuit parameters:
only for Pt 100, with measuring insert Ø6

- Input
- U_i = 60 V
- I_i = 100 mA
- P_i = 192 mW / 290 mW
- C_i = 780 pF/m
- L_i = 0,6 µH/m



WARNING



The device must be installed in a housing that meets the degree of protection against intrusion of at least IP 20. The casing of the measuring insert is not separated from the inner intrinsically safe circuit according to the standard EN 60079-11. This information must be taken into account during installation.

- Intrinsically safe version with converter:**
according to built-in converter
- Power supply of converter:**
DC 24 V from source SELV, e.g. INAP 16 and INAP 901
- Other data of converter:** refer to the enclosed manual
- Display:** LED display to loop 4-20mA
other date refer to enclosed manual

Ingress protection pursuant to EN 60529: IP 65

Operation position:
discretionary; the gland shall not be situated upwards

Type of operation: continuous

Sensor weight:
With ball head (Al alloy), adapter 150 mm and nominal length 200 mm approx. 0.71 kg

Applied materials:

Stem tube of measuring insert	steel 1.4541
Extension	steel 1.4541
Head	aluminium alloy painted with polyester
	paint or plastic PPO (phenyl polyoxide)
Sealing of lid of head	oil-resistant rubber
Internal wiring	Cu
Head terminals of terminal board	brass with Ni surface
Connecting items of sensor	stainless steel

OPERATION CONDITIONS

The environment is defined by the group of parameters and their severity grades IE 36 pursuant to EN 60721-3-3 and the following operation conditions.

- Ambient temperature for head and gland of the sensor:**
 - For design without converter -50 °C to 120 °C
 - For design with converter pursuant to type of converter (refer to enclosed converter manual)
 - For design with converter and display pursuant to type of converter and display (refer to enclosed converter manual)

Intrinsically safe measuring inserts can be used in intrinsically safe circuits of group II electrical equipment.

- Relative ambient humidity:**
 - For design without converter 10 to 100 % with condensation, with upper limit of water content 29 g H₂O/kg of dry air
 - For design with converter pursuant to type of converter (refer to enclosed converter manual)
 - For design with converter and display pursuant to type of converter and display (refer to enclosed converter manual)

Atmospheric pressure: 70 to 106 kPa

Maximum speed of flow of liquids:
pursuant to parameters of thermowell used by the customer

Vibrations:

Sensor	with converter		without converter	
	Nominal length L [mm]	110, 140, 170	200, 260	110, 140, 170
Frequency range [Hz]	10 to 500			
Drift amplitude [mm]	0.2	0.15	0.5	0.2
Acceleration amplitude [ms ⁻²]	29.4	19.6	68.7	39.2

Resistance of material of PPO (phenyl polyoxide) head:

Kerosene	partially resistant
Diesel oil	resistant
Benzene	partially resistant
Animal and vegetable oils	resistant
Weak hydrohides	
Strong hydroxides	
Weak acids	
Strong acids	
Sea water	partially resistant
Trichloroethylene	

Resistance of material of lid sealing (oil-sealing rubber):

Alcohol	resistant
Ether	
Benzol	
Petrol	
Ester	
Animal and vegetable oils	
Mineral oil	
Engine oil	
Weak alkali hydrohides	
Strong alkali hydroxides	
Weak acids	resistant
Strong acids	non-resistant
Sea water	resistant
Trichloroethylene	partially resistant

METROLOGICAL DATA

Probe: measuring resistor Pt 100 in connection pursuant to the scheme and table of designs, α = 0.00385 [K⁻¹], tolerance class A or B pursuant to EN IEC 60751

Range of pair temperature differences pursuant to EN 1434: 3 to 180 K

Internal wiring resistance at 20 °C: 0.1 Ω/m

Calculated resistance value of internal wiring of the design without converter is specified on the label of the measuring insert.

Maximum current load of measuring resistor:

- Pt 100 3 mA
- Pt 500 1 mA

Recommended measuring current:

- Pt 100 1 mA
- Pt 500 0,5 mA

Output signal of the converter (linear with measured temperature):

4 to 20 mA (+ digital for HART protocol)

Calibration depth of immersion of the measuring insert of the sensor

for temperature points within range -70 to 250°C:

200 mm (min. 160 mm)

for temperature points above 250°C:

300 mm (min. 260 mm)

The distance of flange of the measuring insert from the level of medium in the calibration bath shall be at least 40 mm at temperatures to 250°C and min. 70 mm at temperatures above 250°C.

Temperature response time pursuant to EN IEC 60751 in whirling water (characteristic value):

without thermowell (separate measuring insert)

τ_{0.5} 6 s

with thermowells pursuant to DIN 43772, shape 4

(L = 100, 140) τ_{0.5} 85 s

τ_{0.9} 250 s

with thermowells pursuant to DIN 43772, shape 4

(L = 200, 260) τ_{0.5} 53 s

τ_{0.9} 115 s

RELIABILITY

Indicators of reliability in operation conditions and conditions of the environment specified herein

- Mean time of operation between failures 96 000 hours (inf. value)
- Expected service life 10 years

DESIGNATION:

Data of head label

- Trademark of the manufacturer
 - Made in Czech Republic
 - Type of resistance sensor, nominal value R_0 / tolerance class / configuration of wires of internal wiring *)
 - Measuring range or set-up converter range
 - Product ordering number
 - Coverage
 - Time code (Serial number for calibrated design, design with tolerance class A, design with converter, EX ia design)
 - Output signal 4 to 20 mA (design with converter)
 - Ambient temperature
 - Mark of non-explosiveness:
 - ⊕ II 1 G Ex ia IIC T5/T6 Ga (Ex ia design) and number of the EU-Type Examination Certificate
 - Mark CE 1026
 - Other data on design with converter
 - o Output signal 4 to 20 mA
 - o CE mark with identification number of the notified person (for design with converter Ex i)
 - o Designation of non-explosiveness and EU-Type Examination Certificate number (for design with converter Ex i)
 - Other data for design with proof of metrological compliance (/M5)
 - o the conformity marking (CE + supplementary metrology marking) and the number of the notified person
 - o EU type examination certificate number TCM 321/12 - 4906
 - o range of temperature difference
 - o serial number /1 a /2 for unambiguous resolution of sensors for inlet and return pipes
 - other data for design /M1, /M2, /M3 a /M4
 - Evaluation certificate. No ZR 141/10-
- *) Configuration of wires of internal wiring is not specified for the converter

Data on label of measuring insert

- Trade mark
 - Sensor type, nominal value R_0 / tolerance class / Configuration of wires of internal wiring *)
 - Time code (Serial number for calibrated design, design with tolerance class A, design with converter, EX ia design, design with proof of metrological compliance)
 - Resistance value of internal wiring (for design without converter)
- *) Configuration of wires of internal wiring is not specified for the converter

Data on converter label

- Trade mark
- Sensor type
- Pre-set temperature range
- Designation of non-explosiveness and number of the EU-Type Examination Certificate
- the conformity marking CE (for converter Ex ia with the number of the notified person)

Data on display

- Trade mark
- Designation of non-explosiveness and EU-Type Examination Certificate number (for design with converter Ex i)
- the conformity marking CE

DELIVERY

Unless agreed otherwise with the customer, each delivery includes

- Delivery note
- Sensor pursuant to the purchase order
- Allen key 1.5mm
- As accessories to sensors, a suitable cable gland can be delivered; it shall be ordered separately pursuant to the catalogue of accessories, type 991. An instruction sheet is delivered with each cable gland

- Suitable thermowells and nipples ordered separately pursuant to the catalogue of accessories, type 991
- Optional accessories to the sensor with programmable converter
 - o Configuration (parameterization) programme pursuant to the required converter
 - o Communication modem (for serial port RS 232C) pursuant to the required converter
- Accompanying technical documentation in Czech
 - o Product manual
 - o Product quality and completeness certificate, which also serves as the warranty certificate
 - o EU Declaration of Conformity
 - for Ex ia design
 - for design with proof of metrological compliance (/M5)

If it is established in the purchase contract or agreed otherwise, the following documentation can be also delivered with the product:

- Declaration of Conformity with purchase order 2.1 acc. to EN 10204
- EU Declaration of Conformity (for design with converter)
- Calibration sheet (for uncertified calibrated design)
- Copy of EU-Type Examination Certificate pursuant to the Directive No 2014/34/EU (ATEX) for Ex ia design
- Copy of EU-Type Examination Certificate
- Copy of Evaluation certificate for design /M1, /M2, /M3 and /M4
- Test report about the seismic and the vibration qualification

CERTIFICATION

- Non-explosiveness Ex ia, EU-Type Examination Certificate pursuant to the Directive 2014/34/EU FTZÚ 21 ATEX 0007X
- Non-explosiveness Ex ia, EU-Type Examination Certificate pursuant to the 2014/34/EU (pursuant to the type of the converter and display)
- Declaration of metrological conformity (MID) in accordance with Module B of Directive No. 2014/32/EU, EU Type Examination Certificate No. TCM 321/12-4906
- Evaluation certificate. No. ZR 114/10-0068

CALIBRATION

It is realized pursuant to TPM 3342-94 and in compliance with EN IEC 60751, usually in three temperature points evenly distributed within the operation range of the sensor or in the points according to the requirement of the customer. Calibration sheets with measured data are issued for calibrated sensors.

PACKING

Both sensors and accessories are delivered in a packing ensuring resistance to the impact of thermal effects and mechanical effects pursuant to controlled packing regulations.

TRANSPORT

The sensors may be transported on conditions corresponding to the set of combinations of classes IE 21 pursuant to EN IEC 60721-3-2 (i.e. by airplanes and trucks, in premises that are ventilated and protected against atmospheric conditions).

STORAGE

The sensors may be stored on conditions corresponding to the set of combinations of classes IE 11/1K3 pursuant to EN IEC 60721-3-1 (i.e. in places with temperature from -5 to 45 °C and humidity from 5 to 95%, without a special threat of an attack with biological agents, with vibrations of small significance and not situated close to sources of dust and sand).

ASSESSMENT OF CONFORMITY PURSUANT TO THE DIRECTIVE 2014/32 EU

Couple sensors are verified pursuant to EN 1434-5.

The sensors are rated products pursuant to the Directive 2014/32 EU of the European Parliament and the Council and EU Declaration of Conformity is issued for them.

The manufacturer performs subsequent verification under EN 1434-5. Subsequent verification is ordered in the department AMS ZPA N. Paka a.s. (ams@zpanp.cz).

For subsequent verification, send the whole couple tied together.


METHOD OF PLACING THE MARK OF ASSEMBLY AND SERVICE ORGANIZATION AND REINSURANCE MARKS

Verified sensors have a self-adhesive label with reinsurance mark. The label is stuck on the terminal board and the sensor head.

After installation on place of use the sensors will be reassured with mounting seal eventually with label, preventing unauthorized manipulation.

After subsequent verification, the sensors will be provided with a self-adhesive label with an official mark. The label will be stuck on the terminal board and the sensor head instead of the original reinsurance mark.

PLACING THE MARK OF ASSEMBLY AND SERVICE ORGANIZATION AND REINSURANCE MARKS

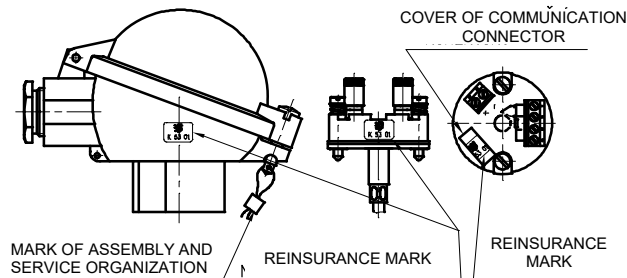

ORDERING TEMPERATURE SENSORS

The purchase order shall specify

- Name
- Product ordering number
- Ex ia design is ordered using codes J4X, D2X or D3X according to table 1
- Additional requirements for sensor design pursuant to Table 2
- Request for other documentation pursuant to Table 2
- Measuring range
- If calibration is required and in what temperature points
- If the delivery of thermowell and nipple pursuant to the type 991 is required for the sensor as accessories
- If the delivery of gland for output cable pursuant to the type 991 is required for the sensor as accessories
- If optional accessories to the sensor with programmable converter is required
- Other (special) requirements
- Number of pieces

Behind the ordering number specified pursuant to the above mentioned table, the customer shall identify the required range of measured temperature (i.e. lower and upper temperature limits in °C) and, as the case may be, other non-standard required parameters for converter configuration (e.g. indication of sensor tripping, dampening, required designation - tagging etc.).

PURCHASE ORDER EXAMPLE

Standard design:

Resistance temperature sensor to thermowell DIN with connecting screw-joint on adapter without converter
236 410 511B/J4/Q1
Calibration points of 100, 250 and 400 °C
range -70 to 600°C
6 pcs

Special requirement:

Resistance temperature sensor Ex d (Ex t) to thermowell DIN with connecting screw-joint on adapter with converter
235 910 511B/18/2.1
nominal length L 380 mm
range 0 to 100°C
6 pcs

ORDERING ACCESSORIES

The purchase order shall specify:

- Name
- Product ordering number
- Number of pieces

PURCHASE ORDER EXAMPLE

Standard design:

1. Welding thermowell pursuant to DIN, shape 4
991 DIN 407544
20 pcs
2. Nipple
991 NVP4 M27 72
6 pcs

Special request:

Nipple
991 NVP4 D27 99
material 1.5415
6 pcs

TABLE 1 - DESIGN OF TEMPERATURE SENSORS TO THERMOWELL DIN, TYPE 235

SPECIFICATIONS						ORDERING NUMBER															
						235	x	x	x	x	x	x	x	x	x	x	/xxxxxx	/xx			
Nominal length L [mm]	110	Length of adapter L _n [mm]	140 (135) ***	Length of measuring L _{mv} [mm] ****	275	1															
	140		150 (135) ***		315	2															
	170		140 (135) ***		335	3	1														
	200		150 (135) ***		375	4	(4)														
	260				435	5															
	410				585	6															
	Other (min. 75) *)						9														
Nominal length L [mm]	110	Length of adapter L _n [mm]	80(75) *** (Without connecting screw-joint)	Length of measuring L _{mv} [mm] ****	215	1															
	140				245	2															
	170				275	3	2														
	200				305	4	(3)														
	260				365	5															
	410				515	6															
	Other (min. 75) *)								9												
Length of adapter L _n [mm]	Adapter	150 (140)				1															
		80 (without connecting screw-joint) max. measuring range [°C] -70 to 250				2															
		Other(min. 65) *) **				9															
	Spiral adapter	75 (without connecting screw-joint) max. measuring range [°C] -70 to 250					3														
135						4															
Other(min. 75) *) **						8															
Thermowell material	without thermowell					0															
Connecting thread	1/2-14 NPT											5									
Head of the sensor	Ball (Al alloy) (for converter Ex i with both external and internal terminals)																				
	Ball, plastic (cannot be used for converter Ex i)																				
	Ball with increased lid (Al alloy) without display for converter in lid or with display (for converter Ex i with both external and internal terminals)																				
	Ball, small (Al alloy) (only for terminal board and converters INPAL 420, TH 100, MINIPAQ-HLP)																				
	Other *)																				
Tube of measuring insert [mm]	Ø6 ± 0,1																				
	Ø3 ± 0,1 (only with connecting thread M14 x 1,5)																				
Measuring resistor (probe)	Pt100																				
	Pt 500																				
Tolerance class	A guaranteed only within range to 300°C																	A			
	B																	B			
Terminal board connection	Single - four-wire (1xPt)																	/J4			
	Double- two-wire (2xPt/B)																	B /D2			
	Double - three-wire (2xPt/ 3)																	/D3			
	Single – four-wire	only for Pt 100,																1 1 /J4X			
	Double – two-wire	with measuring insert ø 6, length of																1 1 B /D2X			
Double – three-wire	measuring insert L _{mv} 100 – 3025 [mm]																1 1 /D3X				

TABLE 1 - DESIGN OF TEMPERATURE SENSORS TO THERMOWELL DIN, TYPE 235 (continuation)

SPECIFICATIONS					ORDERING NUMBER																
					235	x	x	x	x	x	x	x	x	x	/xxxxxx	/xx					
Converter (connection for converter: single, double, three or four-wire, pursuant to the converter)	Converter type		Galvanic separation	Ex ia	NFC	Range [°C]															
	Analogue	INPAL 420				-50 to 50													/07		
						-30 to 70													/55		
						0 to 50														/15	
						0 to 100														/18	
						0 to 150														/19	
						0 to 200															/20
						0 to 250															/21
				0 to 400				1											/23		
	Programmable	TH 100																	/TH100		
		TH 100-ex			•														/TH100X		
		TH 200	•																/TH200		
		TH 200-ex	•	•															/TH200X		
		IPAQ-H	•																/IPAQH		
		IPAQ-HX *)	•	•															/IPAQHx		
		MINIPAQ-HLP																	/MINIPAQ		
		APAQ C130			•														/C130		
		IPAQ C202																	/C202		
		IPAQ C202X			•														/C202		
	HART protocol	IPAQ C330	•																/C330		
		IPAQ C330X	•	•															/C330X		
		IPAQ C520	•																/C520		
		IPAQ C520S	*****) •																/C520S		
		IPAQ C520X	•	•															/C520X		
		IPAQ C520XS	*****) •	•															/C520XS		
		IPAQ C530	•		•														/C530		
		IPAQ C530X	•	•	•														/C530X		
		TH 300	•																/TH300		
		TH 300-ex	•	•															/TH300X		
		MESO-H	•																/MESOH		
		MESO-HX *)	•	•															/MESOHx		
		248 HA NA	•																/248HANA		
		248 HA I1	•	•															/248HAI1X		
		644 HA NA	•																/644HANA		
	644 HA I1	•	•											5				/644HAI1X			
Other *)																		/99			
Without converter (for installation of the converter by the customer)																		/00			
LED display to loop 4-20 mA	LED display LPI-01 (only with converter, except converter 644 HANA)																	/LD			
	LED display Ex ia *) (only with converter Ex ia, except converter 644 HAI1X)																	/LDX			
Special design for negative temperatures -196°C *)																		/CT			
Special design for extreme negative temperatures -269°C *)																		/ECT			

Standard design

- *) Only as a special requirement after an agreement with the manufacturer
- **) In case of adapter length below 140 mm (minimum 80 mm), the temperature range is decreased to -70 to 250 °C.
In case of spiral adapter length below 135 mm (minimum 75 mm), the temperature range is decreased to -70 to 250 °C.
- ***) The value in brackets applies to the spring adapter
- ****) The measuring inserts lengths for the spring adapter are not shown
- *****) Functional safety SIL2

TABLE 2 – ADDITIONAL REQUIREMENT FOR DESIGN OF TEMPERATURE SENSORS TO THERMOWELL DIN, TYPE 236

SPECIFICATIONS				CODE	
PROOF OF METROLOGICAL COMPLIANCE	DESIGN OF TEMPERATURE SENSORS	MEASURING RANGE [°C]	USE		
Proof of metrological compliance pursuant to Directive No. 2014/32/EU (MID), Annex MI-004 *)	couple sensors without converter in connection 1xPt100/..1/4 min. length of measuring insert Ø 6 mm = 210 mm min. immersion = 160 mm	0 to 180	application for residential and business premises and for the light industry	/M5	
CALIBRATION (for sensors as described below)	DESIGN OF TEMPERATURE SENSORS	MEASURING RANGE [°C]	USE		
Calibration by TPM 3342-94, in three calibration points evenly distributed in the sensor measuring range for use as part of the customer's measurement assemblies pursuant to Directive No. 2014/32/EU (MID), Annex MI-002 and MI-005 *)	sensors without converter in connection 1xPt100/..1/4 min. length of measuring insert for temperature to 250°C Ø 6 mm = 210 mm for temperature over 250°C Ø 6 mm = 275 mm	-50 to 50	application for residential and business premises and for the light industry	/M1	
		-50 to 100		/M2	
		0 to 200		/M3	
		0 to 250 for sensors with extension lengths shorter than 125 mm (min. 65 mm)		/M4	
		0 to 300 for sensor with measuring resistance in tolerance class A			
0 to 400 for sensors with extension lengths 125 mm and longer, with measuring resistance in tolerance class B					
CALIBRATION	NUMBER OF CALIBRATION POINTS	CALIBRATION RANGE			
Calibration by TPM 3342-94, define calibration points	3	0 to 420 °C	/Q1		
	3	0 to 600 °C	/Q2		
	3	-196 to 100 °C	/Q3		
	3	-50 to 600 °C	/Q22		
	Other	-50 to 600 °C	/Q9		
REQUIREMENT FOR OTHER DOCUMENTATION		USE			
Copy of EU-Type Examination Certificate (pursuant to Directive No. 2014/32/EU)		M5	/MID		
Copy of Evaluation certificate No. ZR 141/10-0068		M1, M2, M3, and M4	/EC		
EU Declaration of Conformity		for design with converter	/EU		
Copy of EU-Type Examination Certificate acc to the 2014/34/EU		for fixed closure and a dust-tight closure	/Exd		
Copy of EU-Type Examination Certificate acc to the 2014/34/EU		for converter and display Ex ia	/Exi		
Declaration of Conformity with purchase order 2.1 pursuant to EN 10204			/2.1		

Specify the code behind ordering number. Define calibration points for codes Q1, Q2, Q3, Q22 and Q9.



WARNING *)
**)

This request can only be selected with measuring insert Ø6 ± 0,1.
This request cannot be selected for design with spiral adapter

TABLE 3 – ACCESSORIES - OVERVIEW OF DESIGNS RECOMMENDED WELDING THERMOWELLS SHAPE 4 (4F) PURSUANT TO DIN 43772, TYPE 991 (order separately)

SPECIFICATIONS				ORDERING NUMBER										
				991	DIN	x	x	x	x	x	x			
Shape 4	pursuant to DIN	Without flange	PN 250			4	0							
	Shape 4F	43772	With flange **)			4	F							
Internal bore [mm]			ø 7					7						
	Internal thread / external ø of thermowell [mm]		1/2 - 14 NPT/ Ø 26						5					
Cone welding thermowell	Nominal length of thermowell L [mm]	110	L1 [mm]	65	L2 [mm]	105							1	
		140		65		135					2			
		170		133		165					3			
		200		65		195					4			
		200		125		195					5			
		260		125		255					6			
		410		275		405					7			
		Other (max. 1200 *)									9			
	Material of thermowell II	1.7335 ***)		Maximum operation temperature [°C]	550									1
1.7380 ***)		580										2		
1.454 ****)1		580										3		
1.4571 ****)		400										4		
1.5415 *) ***)		530												
1.4903 *) ****)		620												
A105, C22.8 or 1.0460 (P250GH) *) ***)		425												
1.4404 *) ****)		550												
Other *)													9	

*) Upon a special request after an agreement with the manufacturer

***) Flange design (shape, PN, DN and material) pursuant to the requirement of the customer

****) Surface treatment of thermowells: preservation with grease - oil

*****) thermowells of these materials are suitable for contact with food

TABLE 3 – ACCESSORIES - OVERVIEW OF DESIGNS RECOMMENDED SCREW-IN THERMOWELLS SHAPE 7 PURSUANT TO DIN 43772, TYPE 991 (order separately)

SPECIFICATION				ORDERING NUMBER										
				991	DIN	K	x	x	x	x	x			
Cone screw-in thermowell	Shape 7 pursuant to DIN 43772		PN 250			K								
	Internal bore [mm]		Ø 7				7							
	External fixing thread		½ - 14 NPT					5						
			¾ - 14 NPT					7						
			1 - 11,5 NPT						8					
			other *)						9					
	Internal thread for sensor		M18 x1.5						2					
			½ - 14 NPT						5					
			other *)							9				
	Nominal length of thermowell L [mm]	L1 [mm]	110									1		
			140									2		
			170										3	
			200										4	
			260 *)										6	
			410 *)										7	
			Other (maximum 1200) *)										9	
			Material of thermowell	maximum operation temperature [°C]	1.7335 *) **)									
	1.7380 *) **)												2	
	1.4541 ****)													3
	1.4571 ****)													4
1.5415 *) **)													5	
1.4903 *) ****)													6	
A105, C22.8 or 1.0460 (P250GH) *) **)													7	
1.4404 *) ****)													8	
Other *) ****)													9	

*) upon a special requirement after an agreement with the manufacturer
 **) surface treatment of thermowells: preservation with grease – oil
 ***) thermowells of these materials are suitable for contact with food

TABLE 4 – ACCESSORIES - OVERVIEW OF DESIGNS RECOMMENDED NIPPLES FOR WELDING THERMOWELLS, TYPE 991 (order separately)

SPECIFICATION				ORDERING NUMBER				
				991	xxx	x	xxx	xx
Nipple pursuant to DIN 43772 for welding thermowell shape 4 pursuant to DIN 43772	Direct nipple				NVD	4		
	Internal bore [mm]		Ø 26				D26	
	Material		15 128.5 **)	550				51
			1.4541	550				72
			1.5415 *) **)	530				50
			1.4903 *)	620				71
			A105, C22.8 or 1.0460 (P250GH) *) **)	425				20
			1.4404 *)	550				73
			Other *)					
			maximum operation temperature [°C]					

*) upon a special requirement after an agreement with the manufacturer
 **) surface treatment of thermowells: preservation with grease – oil

TABLE 5 – ACCESSORIES - OVERVIEW OF DESIGNS RECOMMENDED NIPPLES FOR SCREW-IN THERMOWELLS, TYPE 991 (order separately)

SPECIFICATION				ORDERING NUMBER					
				991	xxx	x	xxx	xx	
Nipple for screw-in thermowells pursuant to DIN 43772 shape 6 a 7	Direct nipple				NVP				
	Oblique (chamfer 45°)				NVS				
	Internal thread	¾ – 14 NPT	PN	160			4	N34	
		Other *)						999	
	Material		1.0308 or 1.0122 **)	300 (only PN 40)				N34	
			15 128.5 **)	550				G34	
			1.4541	550					72
			Other *)	pursuant to material					99
			maximum operation temperature [°C]						

*) upon a special requirement after an agreement with the manufacturer
 **) surface treatment of thermowells: preservation with grease – oil


INSTALLATION AND CONNECTION

SENSOR INSTALLATION

Install the sensors by screwing into the relevant thermowell screwed into the nipple on the piping (technological equipment) or welded into the piping wall. During the installation, torque of 40 Nm is recommended.

With respect to maintaining metrological properties and the longest possible service life, it is not recommended to install the sensors in places with high turbulence of the medium, which is caused e.g. by a rapid transition from a small diameter of the piping to a larger one (when failing to comply with the required shape and dimensions of diffuser behind the flow meter), etc. Recommended distance of the temperature sensor from the installation flange of the flow meter is min. 1 m.

EXAMPLES OF INSTALLATION OF THERMOWELLS DIN

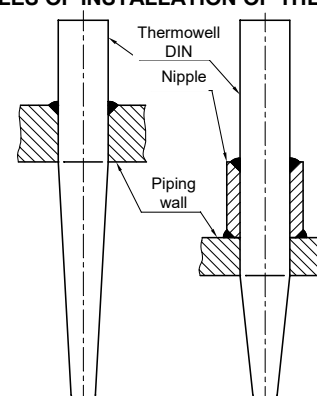

ELECTRICAL CONNECTION

The sensor installation in conditions with explosive gaseous atmosphere or flammable dust shall comply with the requirements of EN 60079-14.

The terminal board of the sensor (converter) is accessible after the removal of the lid of the head.

Connect the evaluation devices to the sensor with a non-armoured cable with double insulation (internal wires with Cu core with cross-section 0.5 to 1.5 mm²).

Seal the cable in the gland by prescribed tightening of the closing nut pursuant to instruction sheet of the gland. Then secure it with clamp against pull-out.

WARNING

Do not use independent wires without jacket for electrical connection. The cable must be circular and compact, the filler or shell must be extruded and the filler material, if used, must be non-absorbent. The length of the connecting cable must be at least min. 3 m. Temperature resistance of the cable shall comply with the ambient temperature!

The cable insulation shall have chemical and mechanical resistances in compliance with the conditions, in which the cable will be installed. It is recommended supporting the cable along its length between the sensor and the follow-up device. In the environment with interfering signals, use shielded cable in the power supply circuit. Shielding may be only grounded (earthed) in one point. The cable should not be placed together with power cables.

In case of the sensor with HART protocol converter, the maximum length of wiring is defined by the arrangement of wires of the connecting cable. The total length of wiring may be up to 1500 m. It requires a twisted two-wire with shared shielding with the diameter of the cross section min. 0.5 mm². The HART communicator is connected to the supply loop of the sensor with converter pursuant to Figure 1.

To achieve reliable communication, the total load resistance of min. 250 Ω shall be in the circuit of the output loop.

INSTALLATION OF THE SENSOR IN ENVIRONMENT WITH EXPLOSIVE GASEOUS ATMOSPHERE

The installation of the sensor in the environment with explosive gaseous atmosphere shall comply with the requirements of EN 60079-14.

The sensor without converter (with ball head from alloy Al with external and internal terminals – only on ZP (special requirement) after an agreement with the manufacturer) can be used as a simple device pursuant to EN 60079-11 Article 5.7 in an intrinsically safe circuit Ex ia pursuant to EN 60079-25. For a simple device, the maximum temperature can be determined from the value of the P0 of the connecting device and the temperature class is determined.

The sensor with converter Ex ia may be used in case of compliance with the parameters Ex ia of the converter according to the enclosed converter manual.

Only insulated cables must be used in intrinsically safe circuits which is able to withstand the electrical strength test with a voltage equal to twice the voltage in the intrinsically safe circuit, or 500 V eff (DC 750 V), taking greater of the values.

In case of installation of intrinsically safe circuits, including cables, the maximum permitted inductance, capacity or ratio L/R and surface temperature may not be exceeded. Permitted values can be found out in the documentation of the follow-up equipment or label with the designation. Locate the follow-up equipment outside of the dangerous area. An intrinsically safe source must be always used that is approved for power supply of intrinsically safe equipment in the sense of EN 60079-11. If a LED display is required, it must be in the design Ex ia.

WARNING


The programmable converter may not be connected to the PC or HART communicator if the converter is located in the explosive environment.

Shielding of the cable of the intrinsically safe circuit must be grounded in the same place as the intrinsically safe circuit, the connection must be outside the dangerous area

For the installations in dangerous areas, mutual interconnection is required (bringing to the same potential). To achieve it, terminals on the sensor head can be used.

The sensor need not be connected to the system of mutual interconnection separately if it is installed firmly and has metal interconnection with the structural parts or the piping, which is connected to the system of mutual interconnection.

HEAD OF THE SENSOR WITH TERMINALS
(for sensor with converter Ex i)

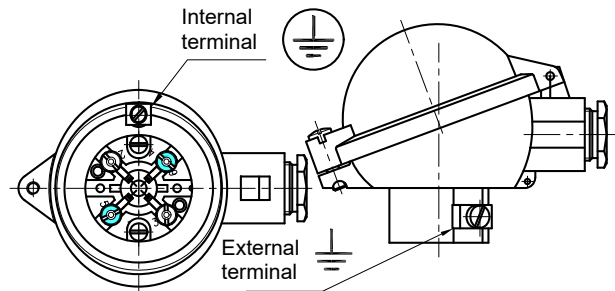

Maximum cross-section of wire for connection to external and internal terminals:

Internal terminal: stranded wire 1.5 mm², full wire 2.5 mm²
External terminal: stranded wire 4.0 mm², full wire 6.0 mm²
If stranded wires are used for the interconnection, they shall be protected against fraying with pressing hollow.

COMMISSIONING

After the sensor installation, including the fixed closure, and connection of the follow-up (evaluation) device to the supply voltage (and the settlement period of the converter), the equipment is prepared for operation.

WARNING

After installation must be require initial inspection equipment and installations according to EN 60079-17



OPERATION AND MAINTENANCE

The sensor does not require any operation; maintenance and follow-up regular periodic revision or permanent supervision of expert staff are performed pursuant to EN 60079-17

SENSOR UNINSTALLATION

Disconnect the sensor from the power supply source. The terminal board of the sensor (converter) is accessible after tilting away the lid of the head, which is connected with one screw.

The measuring insert of the sensor is replaceable and is uninstalled from the head after disconnecting the cable by releasing two screws.

If the sensor is connected to the system of interconnection, the wire for mutual interconnection shall be released from the terminal on the head of the sensor before the complete uninstallation of the sensor.

Unscrew the sensor from the thermowell, torque for releasing is approx. 40 Nm. When releasing the screw joint of the sensor, the thermowell may never be released.

SPARE PARTS

Spare parts shall be delivered by the manufacturer. Relevant measuring inserts can be ordered pursuant to the following table (the table applies only to the version without a spring adapter):

SPECIFICATION		ORDERING NUMBER					
		MV230	/xxx/	1	x	x	/xxxx
Length of measuring insert [mm]			pursuant to tab. 1	1			
Sensing probe	Pt100				1		
	Pt500				2		
Tolerance class	A					A	
	B					B	
Connection of terminal board or converter	Pt100/ /4						/J4
	2xPt100/B/2					B	/D2
	2xPt100/ /3						/D3
	Pt/ /4 *)			1	1		/J4X
	2xPt/B/2 *)			1	1	B	/D2X
	2xPt/ /3 *)			1	1		/D3X
Converter pursuant to tab. 1							/converter

*) Ex ia design

PURCHASE ORDER EXAMPLE OF MEASURING INSERT

Resistor measuring insert without converter
230 /375/ 11B/J4
6 pcs

To order the certified measuring inserts, specify the code according to Table 2 – Additional requirements – behind the ordering number.

The measuring inserts are marked according to Article DESIGNATION. Designation is completed with the ordering number.

Each delivery includes

- Delivery note
- Measuring insert pursuant to the purchase order
- Optional accessories to the measuring insert with a programmable converter
 - o Configuration program according to the required converter
 - o Communication modem (for serial port RS 232C) according to the required converter
- Accompanying technical documentation in Czech
 - o Product manual
 - o Product quality and completeness certificate, which also serves as the warranty certificate
 - o EU Declaration of Conformity (for Ex ia design)

If it is established in the purchase contract or agreed otherwise, the following documentation can be also delivered with the product

- Calibration sheet (for calibrated design)
- Declaration of Conformity of the supplier according to EN ISO/IEC 17050-1
- Copy of EU-Type Examination Certificate pursuant to the Directive No 2014/34/EU (ATEX). for Ex ia design

WARRANTY

The warranty period is 24 months from the receiving of the product by the customer, unless established otherwise in the contract. Rejection of defects shall be enforced in writing at the manufacturer within the warranty period. The rejecting side shall identify the product name, ordering and manufacturing numbers, date of issue and number of the delivery note, clear description of the occurring defect and the subject of the claim. If the rejecting side is invited to send the device for repair, it shall do so in the original package of the manufacturer and/or in another package ensuring safe transport.

The warranty shall not apply to defects caused by unauthorized intervention into the device, its forced mechanical damage or failure to comply with operation conditions of the product and the product manual.

REPAIRS

The sensors shall be repaired by the manufacturer. They shall be sent for repair in the original or equal package without accessories.

DISABLING AND LIQUIDATION

The product and its package do not include any parts that could impact the environment.

Products that are withdrawn from operation, including their packages (with the exception of products marked as electrical equipment for the purposes of return withdrawal and separate salvage of electrical waste), may be disposed of to sorted or unsorted waste pursuant to the type of waste.

The manufacturer realizes free return withdrawal of marked electrical equipment (from 13.8.2005) from the consumer and points out the danger connected with their illegal disposal. The package of the sensor can be recycled completely. Metal parts of the products are recycled, non-recyclable plastic materials and electrical waste shall be disposed of in accordance with applicable legislation.

FIGURE 1- EXAMPLE OF OPERATION CONNECTION OF TEMPERATURE SENSOR WITH CONVERTER IN LOOP 4 - 20 mA


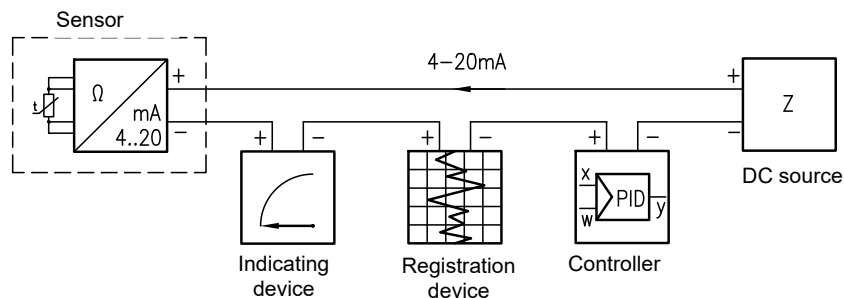



FIGURE 2 – SCHEME OF CONNECTION OF TEMPERATURE SENSORS

SCHEME OF CONNECTION WITHOUT CONVERTER


J4 - With simple measuring resistor in four-wire connection (Pt 100/ /4)



D2 - With double measuring resistor in two-wire connection (2 × Pt 100/B/2)



D3 - With double measuring resistor in three-wire connection (2 × Pt 100/ /3)

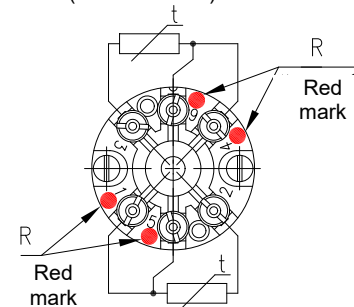

SCHEME OF CONNECTION WITH CONVERTER AND DISPLAY


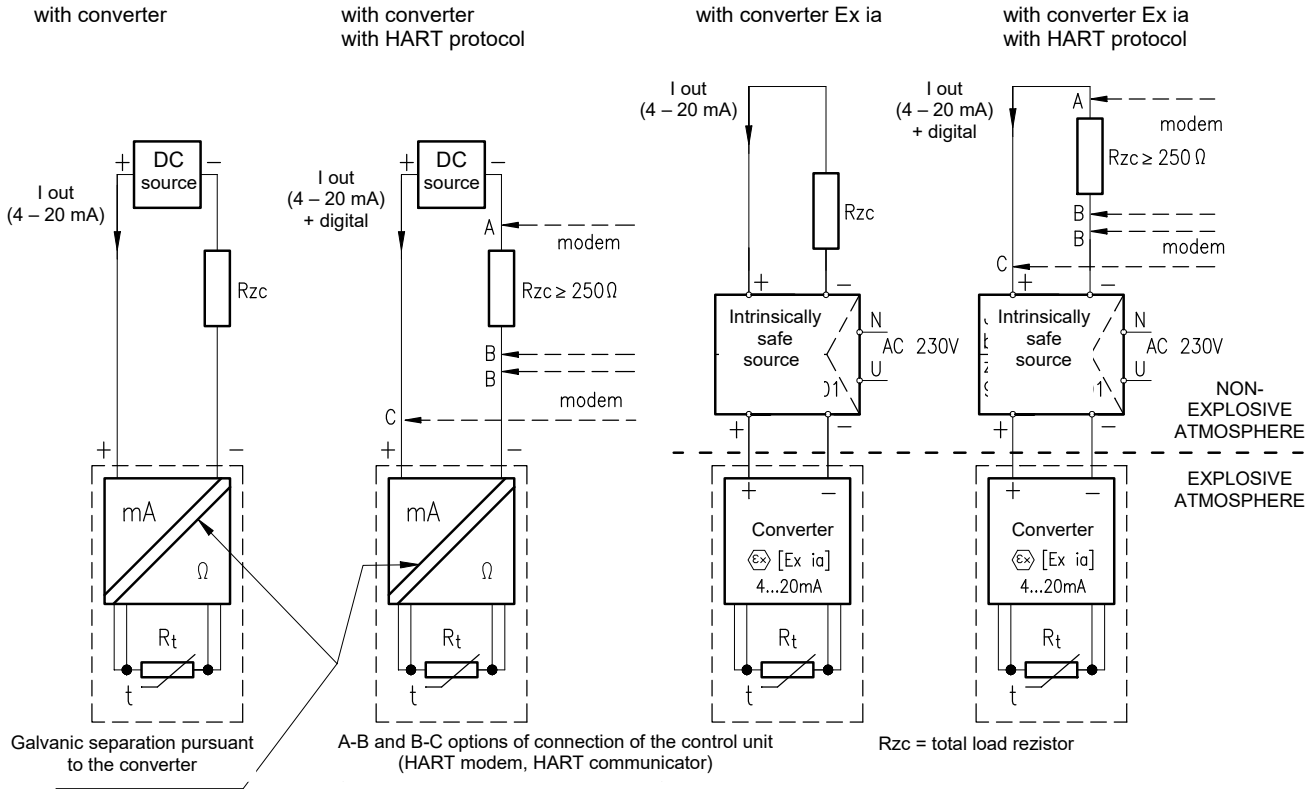


FIGURE 3 - INTRINSICALLY SAFE MARKING



April 2023
© ZPA Nová Paka, a.s.

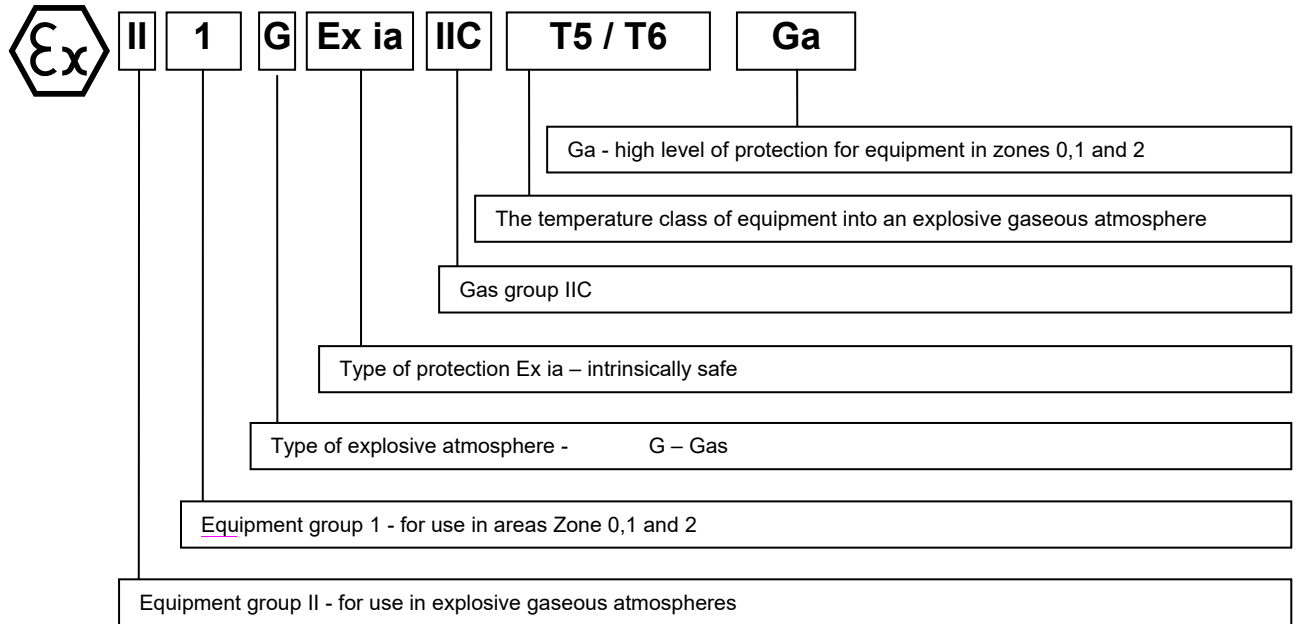

ZPA Nová Paka, a.s.
Pražská 470
509 01 Nová Paka

tel.: spojovatel: 493 761 111
e-mail: obchod@zpanp.cz
www.zpanp.cz

bankovní spojení: ČSOB HK
číslo účtu: 271 992 523/300

IČO: 46 50 48 26
DIČ: CZ46504826